



File D:\DATA\SHYY\MONITOR\MJ-772-T-11165-LCMSA044.D

Injection Date : 26 Nov 25 9:59 am +0800 Tgt Mass(EZX) : 550.00
Sample Name : MJ-772-T Location : P1-A-02
Acq. Operator : SHYY-MONITOR Inj : 1
Spec. Reported : MS Integration Inj Volume : 2 ul
Acq. Method : D:\METHODS\1-POS-5MIN.M
Analysis Method : D:\METHODS\1-POS-5MIN.M
Sample Info : Easy-Access Method: '1-POS-5MIN' 550.00
Method Info : Mobile Phase: A: water(0.01%TFA) B: ACN(0.01%TFA)
Gradient: 5%-95% B in 2.5min
Flow Rate: 1.8 ml/min
Column: Poroshell 120 C18 4.6*50mm, 4um
Oven Temperature: 45 C
UV214, MASS110-1500


*DAD1 A, Sig=214,4 Ref=off

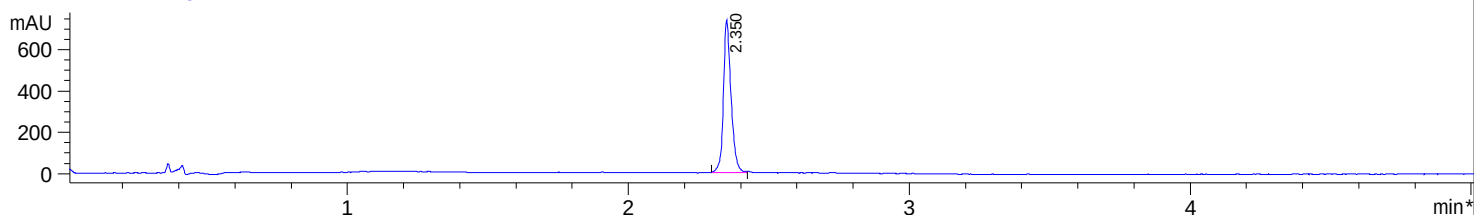


*DAD1 B, Sig=254,4 Ref=off

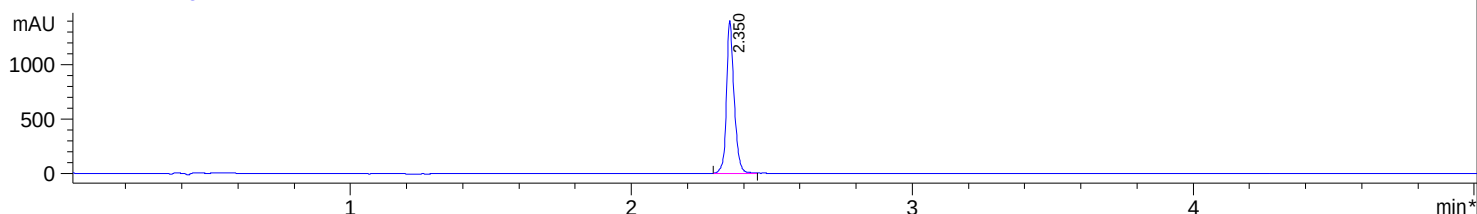

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

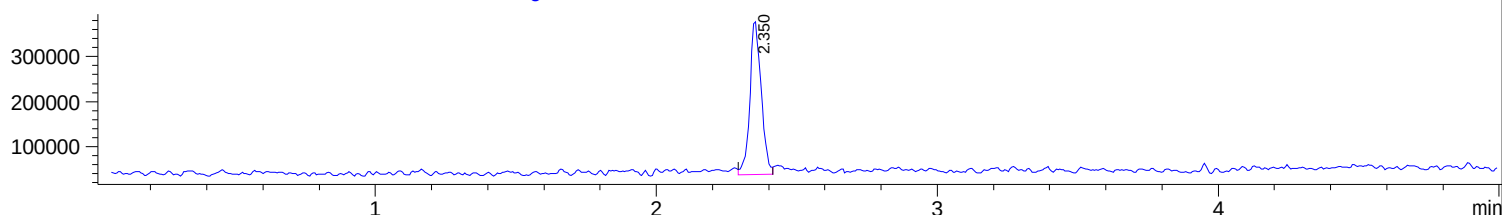

Ion 551, MSD1 551, Target Mass 550 +H Positive, EIC=550.7:551.7

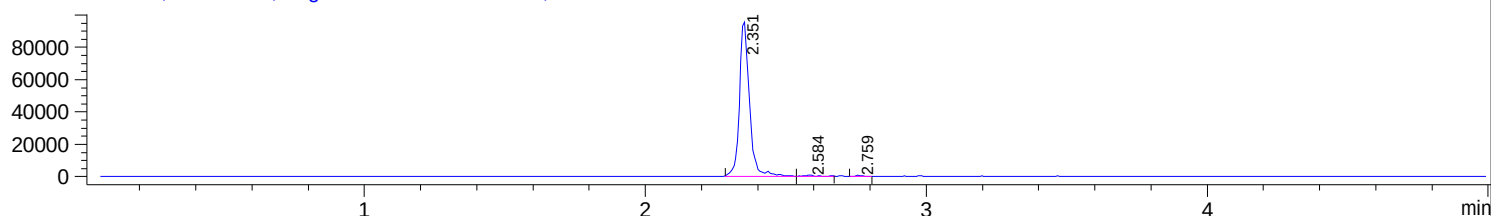

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
2.35	0.03	1389.48	739.08	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
2.35	0.03	2635.80	1407.02	100.00

Ret. Time: 2.35

<<<< POSITIVE SPECTRA >>>>

