

7.349
7.330
7.261
7.236
7.210
7.175
7.157
7.099
7.079
7.006
6.987
6.968

4.005
3.989
3.973


2.509
2.337
2.323
2.174
1.779
1.763
1.747

Current Data Parameters
 NAME 11-15-2022
 EXPNO 62
 PROCNO 1

F2 - Acquisition Parameters
 Date_ 20221203
 Time 12.33
 INSTRUM spect
 PROBHD 5 mm PABBO BB-
 PULPROG zg30
 TD 65536
 SOLVENT DMSO
 NS 16
 DS 2
 SWH 8223.685 Hz
 FIDRES 0.125483 Hz
 AQ 3.9846387 sec
 RG 138.14
 DW 60.800 usec
 DE 6.50 usec
 TE 292.1 K
 D1 1.00000000 sec

===== CHANNEL f1 =====
 NUC1 1H
 P1 13.40 usec
 PLW1 16.00000000 W
 SFO1 400.1324710 MHz

F2 - Processing parameters
 SI 65536
 SF 400.1300000 MHz
 WDW EM
 SSB 0
 LB 0.30 Hz
 GB 0
 PC 1.00

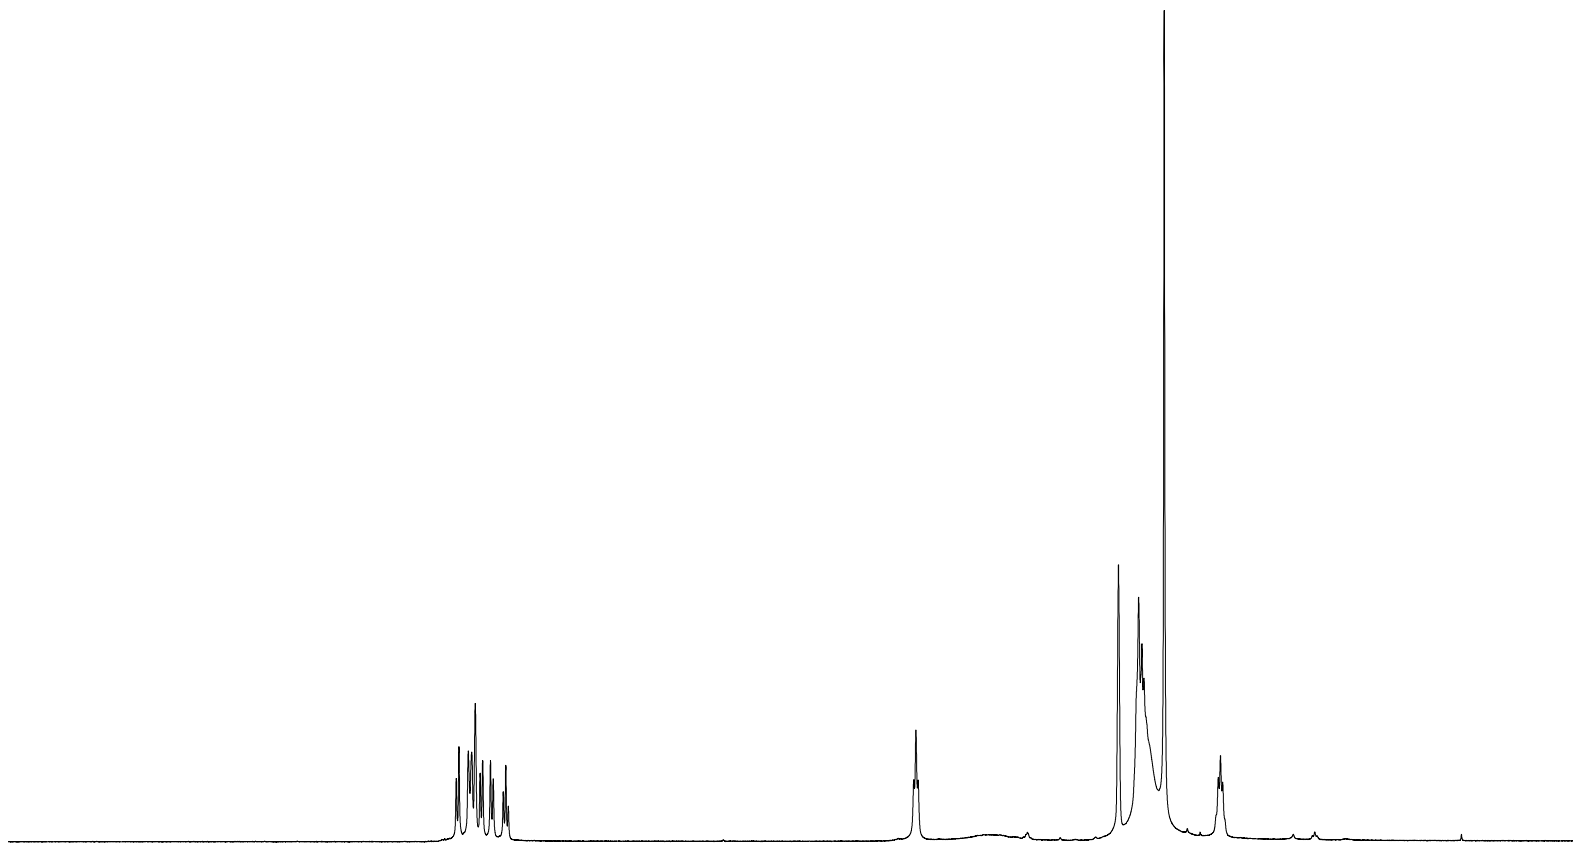

10 9 8 7 6 5 4 3 2 1 0 ppm

1.03
3.00
1.02
1.05
1.01

2.01

12.90
6.16
2.02