

Control Method: C:\GILSON\UNIPPOINT\SYSTEM.GCT
 Analysis Method: C:\GILSON\UNIPPOINT\SYSTEM.GAN
 Sample name: mt-cc006-499 Sample site: Sample:47
 Channel Scales
 <Auto range Analysis Channel>


Injection Number: 86

214 0.00 to 10.00 mVolt (0 %offset), Data rate: 20.00 (points/second) *Unknown*
 254 0.00 to 10.00 mVolt (5 %offset), Data rate: 20.00 (points/second)

Peak Table <Auto zero> <Analysis Channel>
 <None> <Auto zero>

Peak Detection Parameters

Relative Error: 5 (%) Absolute Error: 0.1 (min)

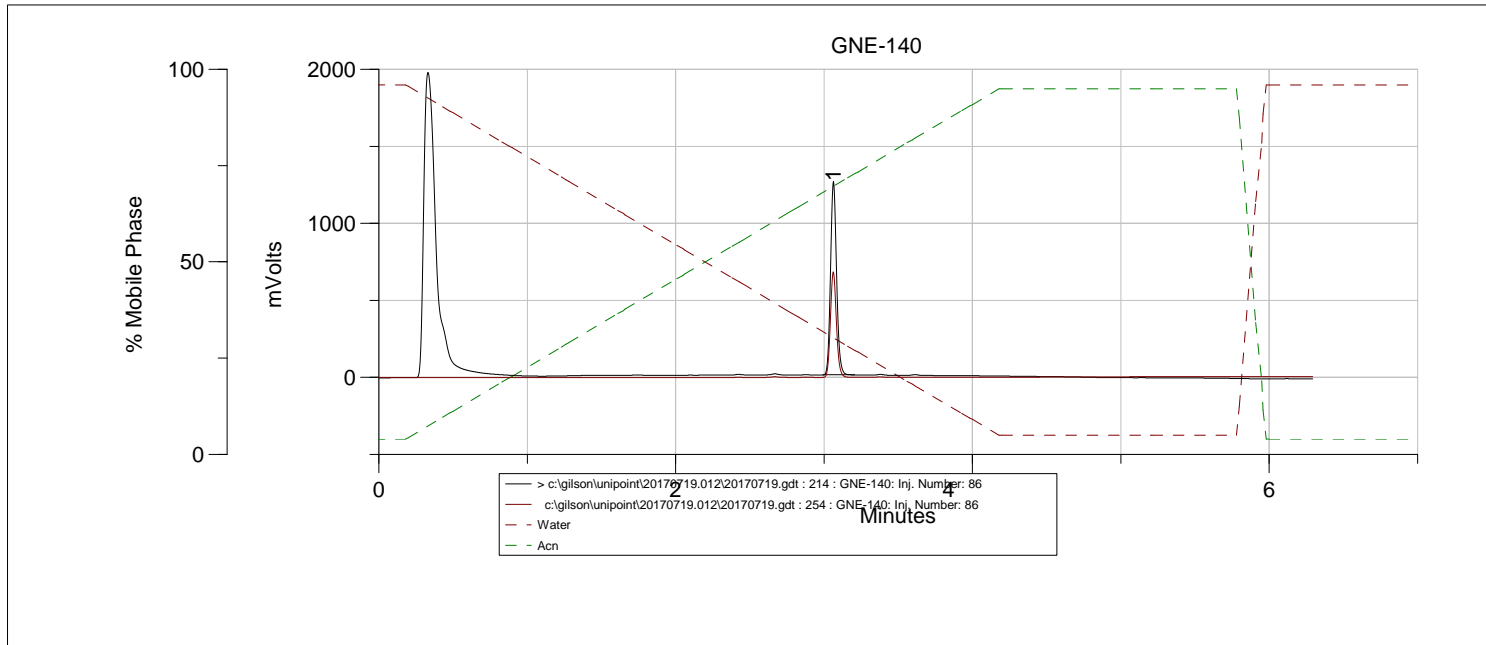

	Inj. Number	Peak Name	Sample Descrip.	R. Time	Sample Location	Height	Area	Area %		
1	86.00	1	GNE-140	3.06	Sample:47	1255.13	5895366.50	100.00		