


## HPLC Result

### Injection Details

Injection Name:	PC-5000801	Run Time (min):	46.00
Vial Number:	RC4	Injection Volume:	2.00
Injection Type:	Unknown	Channel:	UV_VIS_1
Calibration Level:		Wavelength:	214.0
Instrument Method:	GDL 0-30min ACN2%-90% with wash and baseline	Bandwidth:	4
Processing Method:	Processing Method	Dilution Factor:	1.0000
Injection Date/Time:	21/SEP/18 10:30	Sample Weight:	1.0000

### Chromatogram

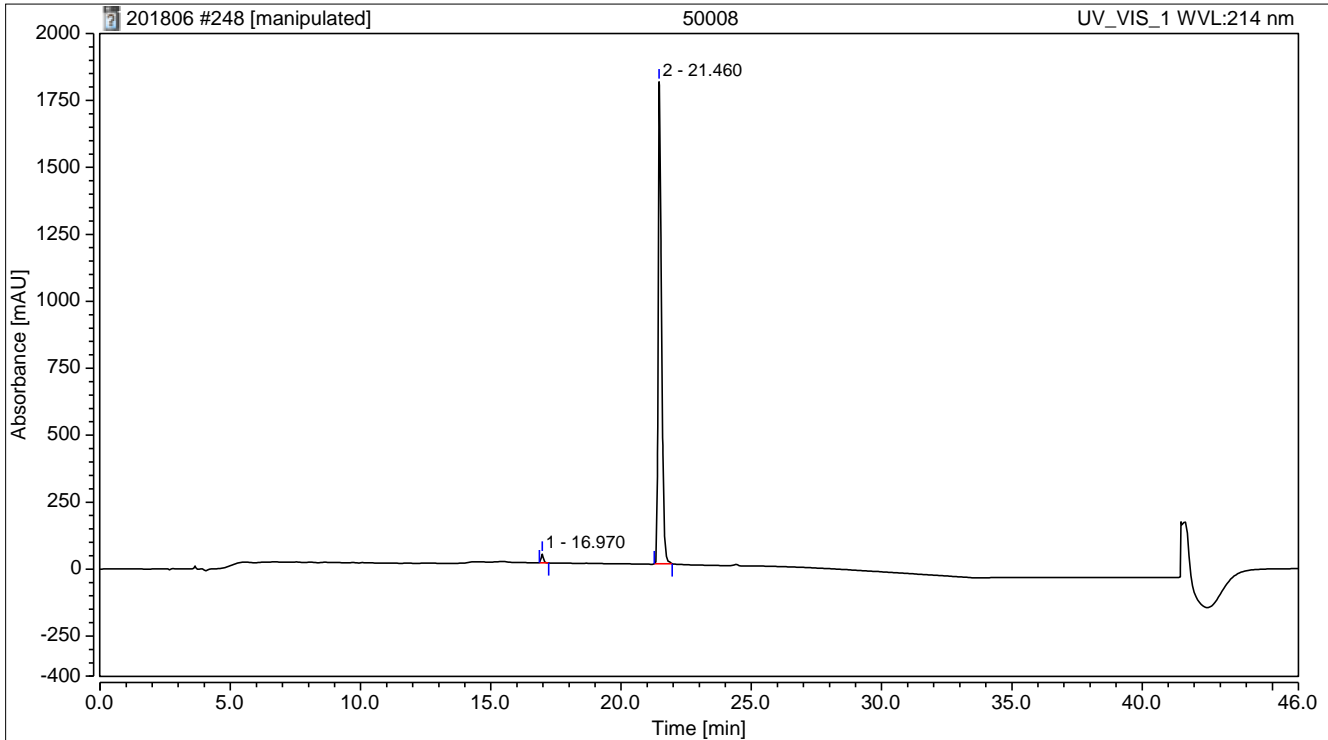

### Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount n.a.
1		16.970	3.065	32.837	1.11	1.79	n.a.
2		21.460	272.343	1799.652	98.89	98.21	n.a.
Total:			275.408	1832.489	100.00	100.00	