


Instrument:HPLC Sequence:20180402

Chromatogram and Results

Injection Details

Injection Name:	PC-61030	Run Time (min):	1.50
Vial Number:	RC7	Injection Volume(L):	1.0
Injection Type:	Unknown	Polarity	
Instrument Method:	Base(POS)-1.5min		
Processing Method:	Default		
Injection Date/Time:	08/Apr/18 09:52		

Chromatogram

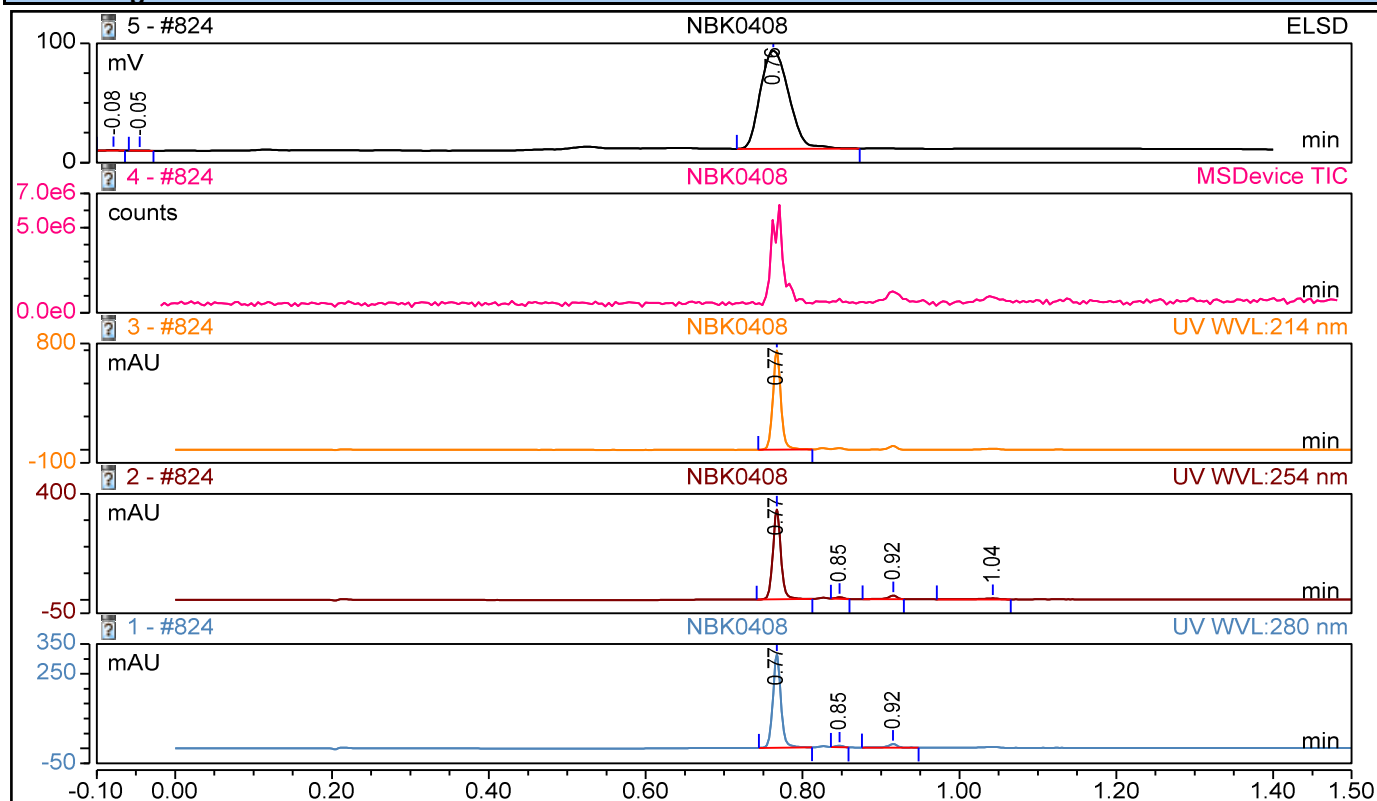

Integration @ 214nm

Peak No.	Retention Time min	Area mAU*min	Rel.Area %	Height mAU	Peak Purity
1	0.77	8.747	100.00	746.79	1000

Integration @ 254nm

Peak No.	Retention Time min	Area mAU*min	Rel.Area %	Height mAU	Peak Purity
1	0.77	3.945	91.38	337.76	1000
2	0.85	0.065	1.51	6.14	992
3	0.92	0.189	4.38	13.79	996
4	1.04	0.118	2.72	4.05	962

Integration @ 280nm

Peak No.	Retention Time min	Area mAU*min	Rel.Area %	Height mAU	Peak Purity
1	0.77	3.642	94.03	311.86	1000
2	0.85	0.052	1.34	4.83	993
3	0.92	0.179	4.63	12.10	991

Mass and UV Spectrum of Peaks integrated @ 214nm

