


MS Report

Sample Name:	PC-6118201 -MS BD8	Injection Volume:	1.0
Vial Number:	unknown	Channel:	UV_VIS_1
Sample Type:	PH-45V	Mass Range:	n.a.
Control Program:	AAA	Polarity:	n.a.
Quantif. Method:	5/24/2018 13:47	Dilution Factor:	1.0000
Recording Time:	2.50	Sample Weight:	1.0000
Run Time (min):		Sample Amount:	1.0000

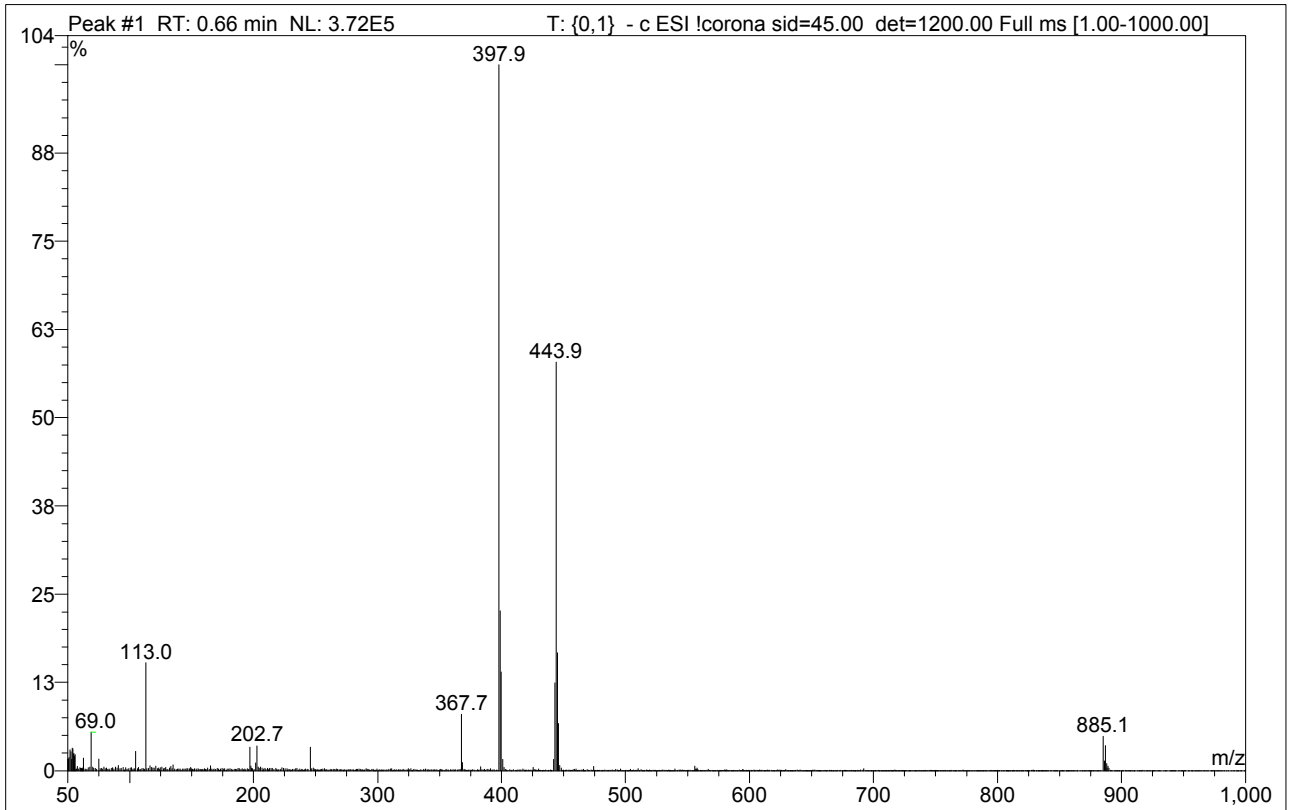

No.	Ret.Time min	Peak Name	Base Peak amu	Int. Base counts	Peak 1 amu	Peak 2 amu	Peak 3 amu	Int. Peaks delta%
1	0.19	n.a.	104.9	9346.0	n.a.	n.a.	n.a.	n.a.
<b>Average delta% from expected Intensity:</b>								<b>n.a.</b>