


Acq. Method : D:\METHODS\1-POS-3MIN.M
 Analysis Method : D:\METHODS\1-POS-3MIN.M
 Sample Info : Easy-Access Method: '1-POS-3MIN'
 Method Info : Mobile Phase : A:water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient:5% increase to 95%B within 1.3min,95%B for 1.7min
 Flow Rate :2ml/min
 Column :Sunfire, 50*4.6mm,3.5um
 Column Temperature:50C
 Detection:UV(214,4nm) and MS(ESI,Pos mode,110 to 1000 amu)

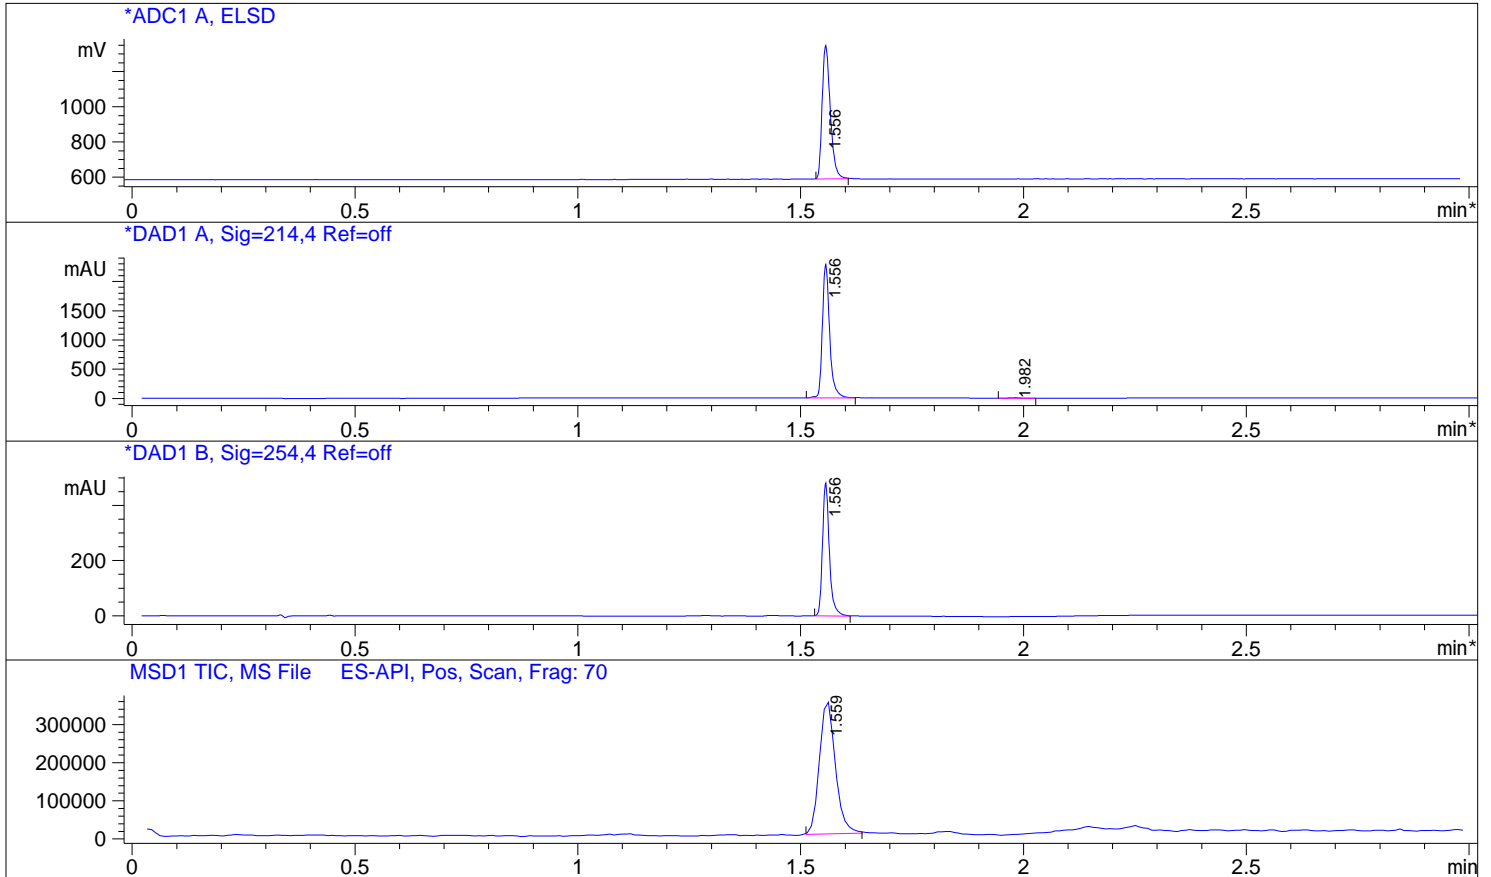

Integration Results for ADC1 A, ELSD

RetTim	Width	Area	Height	Area%
1.56	0.02	962.30	759.72	100.00

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
1.56	0.02	2583.97	2288.38	99.33
1.98	0.02	17.48	10.27	0.67

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
1.56	0.02	517.37	482.83	100.00

Ret. Time: 1.56

<<<< POSITIVE SPECTRA >>>>

