


HPLC Report

Injection Details

Injection Name:	DBET6-pure	Run Time (min):	46.00
Vial Number:	GD1	Injection Volume:	2.00
Injection Type:	Unknown	Channel:	UV_VIS_2
Calibration Level:		Wavelength:	214.0
Instrument Method:	GDL 0-30min ACN2%-90% with wash and baseline	Bandwidth:	4
Processing Method:	Processing Method	Dilution Factor:	1.0000
Injection Date/Time:	30/Oct/18 09:43	Sample Weight:	1.0000

Chromatogram

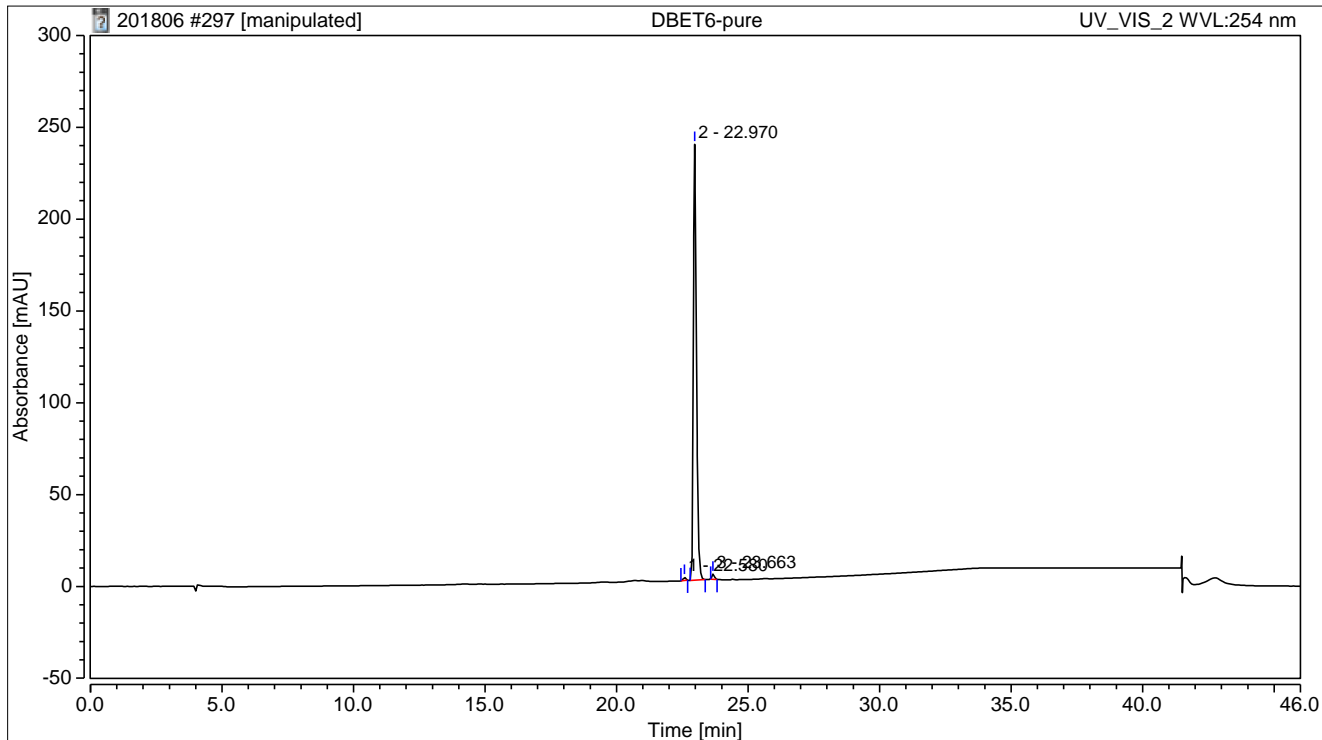

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount n.a.
1		22.580	0.200	1.782	0.61	0.74	n.a.
2		22.970	32.355	237.375	98.46	98.11	n.a.
3		23.663	0.307	2.782	0.93	1.15	n.a.
Total:			32.862	241.939	100.00	100.00	