


## HPLC Result

### Injection Details

Injection Name:	PC-7015801	Run Time (min):	46.00
Vial Number:	RA8	Injection Volume:	2.00
Injection Type:	Unknown	Channel:	UV_VIS_1
Calibration Level:		Wavelength:	214.0
Instrument Method:	GDL 0-30min ACN2%-90% with wash and baseline	Bandwidth:	4
Processing Method:	Processing Method	Dilution Factor:	1.0000
Injection Date/Time:	19/Sep/18 13:17	Sample Weight:	1.0000

### Chromatogram

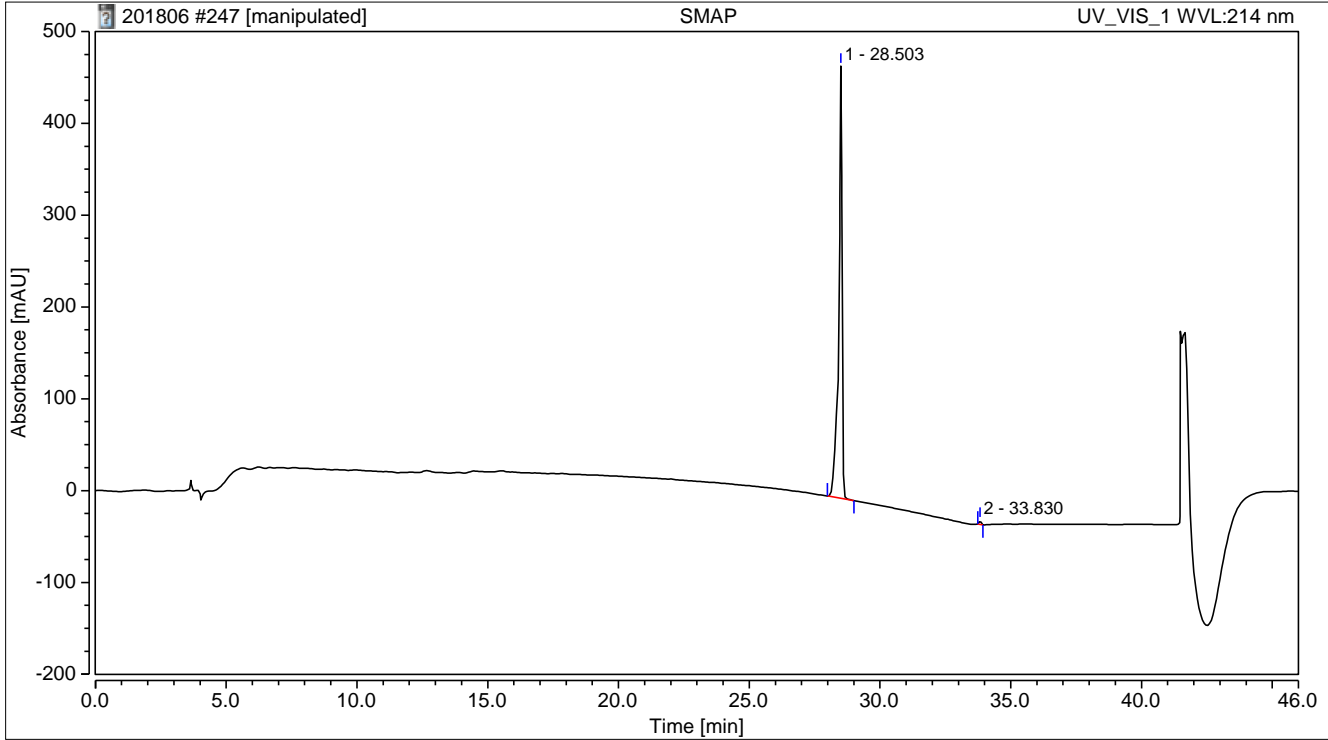

### Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount n.a.
1		28.503	66.365	470.729	99.43	99.03	n.a.
2		33.830	0.381	4.616	0.57	0.97	n.a.
Total:			66.746	475.345	100.00	100.00	